
Nicolet Viking IV [redacted] [redacted]

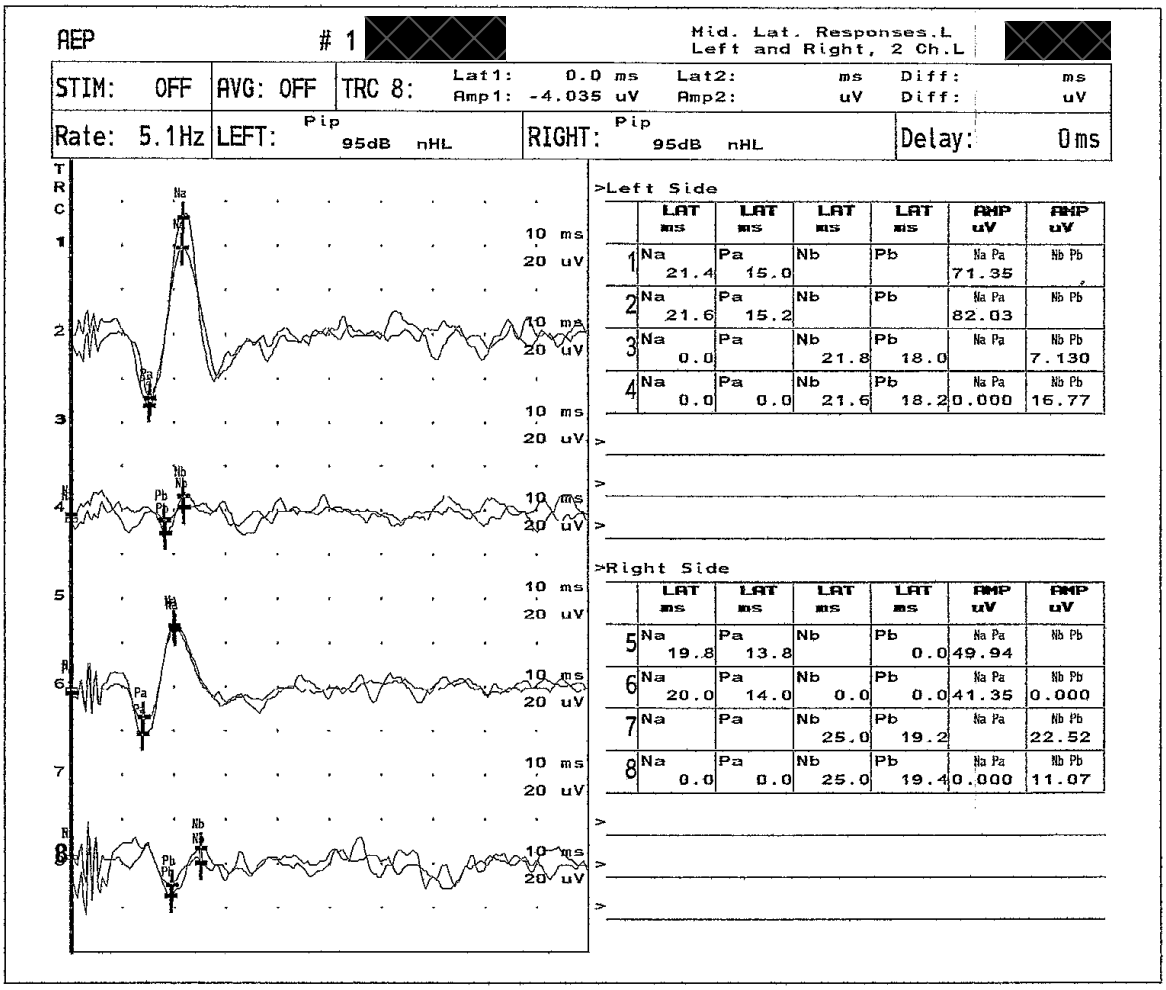


Vestibulo myography Testing
Type of test: T. Pip MLR 2Ch normal average.
Test ear (L) L- 90 dB R-30 dB nHL Noise Off.
Frequency 750 Hz
Reject. Off.
Settings. LFF 20Hz
HFF 1.5Hz
Average 100
Stim. Rate 5.1Hz
DSNS: 20 µV/d
Time base 10 ms

Indication: Imbalance, Dizziness, DX- CP